Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15600	**Temperature:**	23.5 °C
Model:	KICHER PR	**Humidity:**	43%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


410.2 mv/5000g
(82.0 µv/g)
R^2: 0.999961 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 1 1 2026

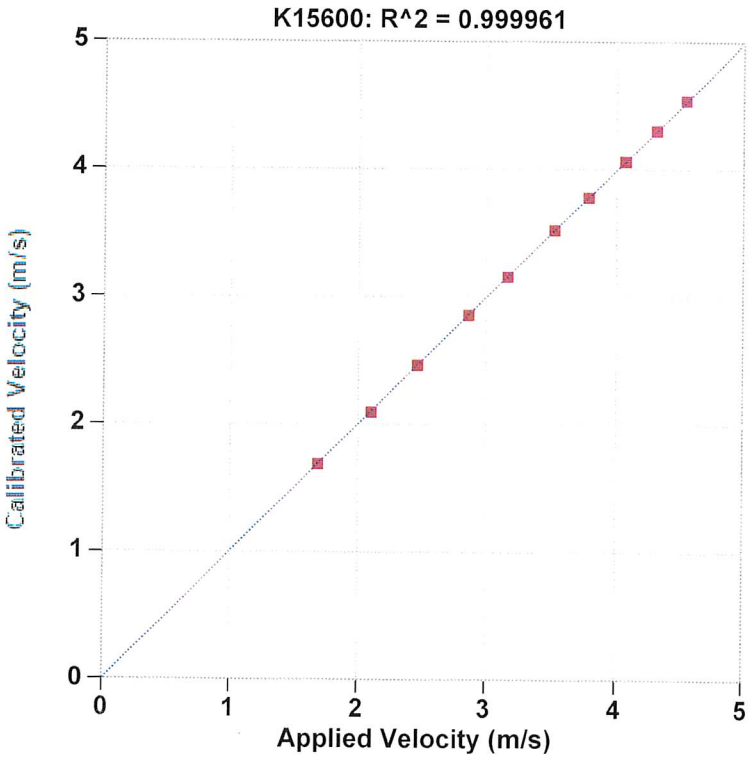

Reference Velocity	S/N K15600 Velocity
m/s	m/s
1.687	1.685
2.101	2.093
2.463	2.462
2.861	2.857
3.165	3.158
3.525	3.523
3.783	3.783
4.065	4.064
4.302	4.306
4.531	4.544

Maximum Acceleration: 970 g's