Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15635	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	28%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


429.3 mv/5000g
(85.9 µv/g)
R^2: 0.999991 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

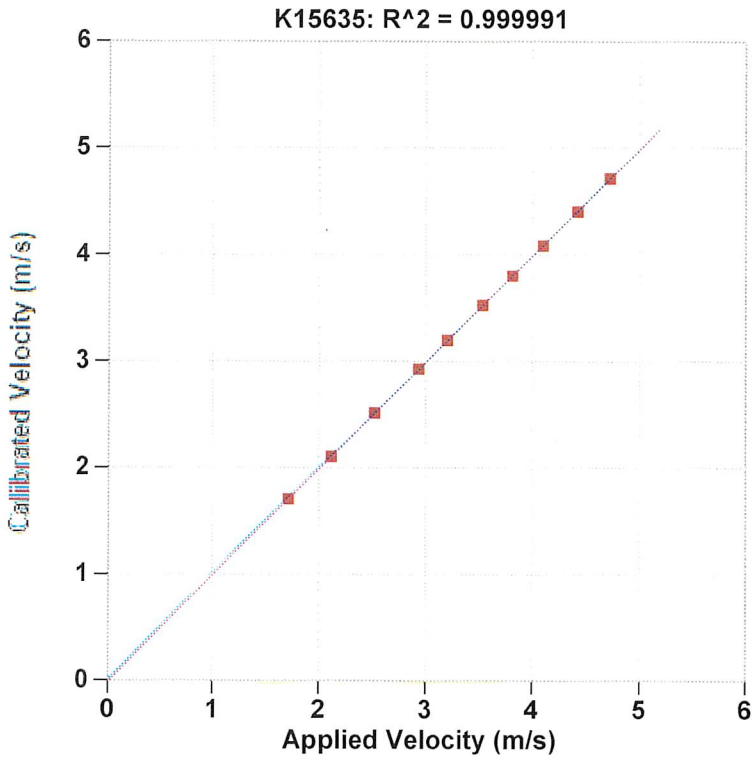

Reference Velocity	S/N K15635 Velocity
m/s	m/s
1.712	1.712
2.106	2.110
2.511	2.516
2.924	2.927
3.197	3.199
3.530	3.530
3.809	3.807
4.092	4.090
4.413	4.409
4.721	4.722

Maximum Acceleration: 1067 g's