Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15636	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	28%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

416.4 mv/5000g
(83.3 µv/g)
R^2: 0.999994 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

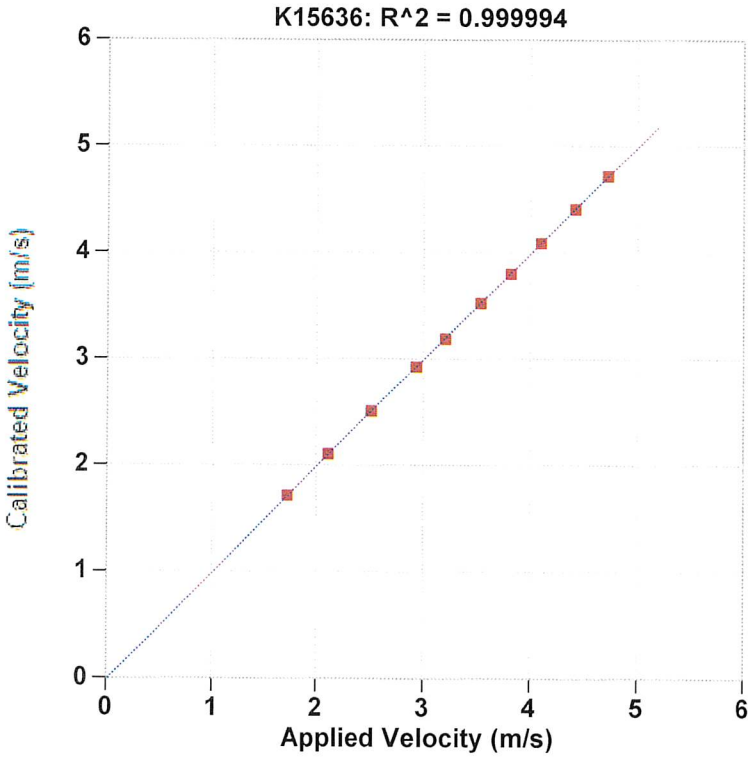

Reference Velocity	S/N K15636 Velocity
m/s	m/s
1.712	1.716
2.106	2.107
2.511	2.512
2.924	2.924
3.197	3.193
3.530	3.528
3.809	3.805
4.092	4.093
4.413	4.414
4.721	4.724

Maximum Acceleration: 1067 g's