Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15640	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	28%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85363! 1000 g's/volt	**Cal on:**	14Nov2025
Ref Acc 2:	85382! 958 g's/volt	**Cal on:**	24Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

416.5 mv/5000g
(83.3 µv/g)
R^2: 0.999973 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

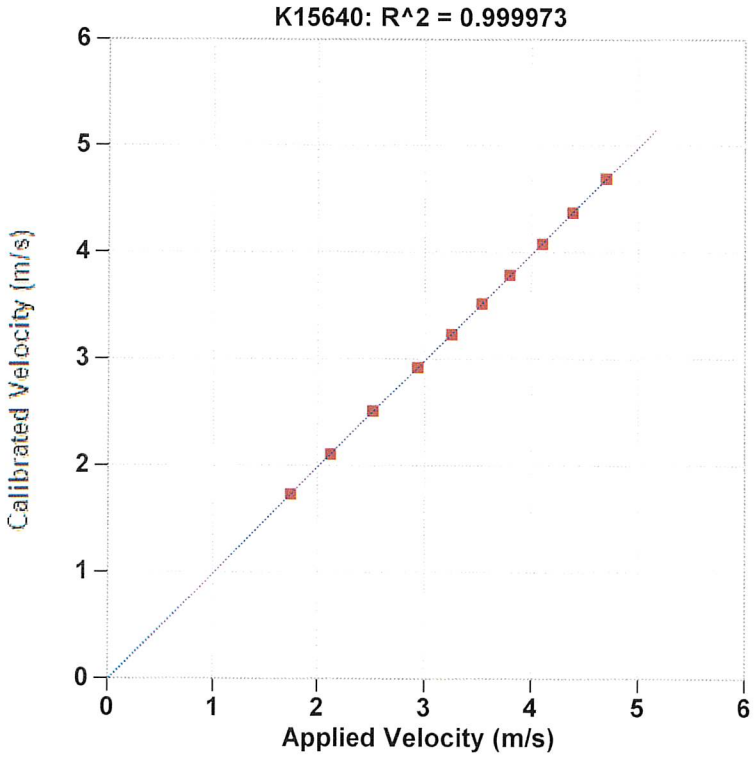

Reference Velocity	S/N K15640 Velocity
m/s	m/s
1.735	1.732
2.115	2.109
2.515	2.518
2.924	2.925
3.242	3.239
3.526	3.525
3.789	3.796
4.096	4.087
4.384	4.385
4.695	4.701

Maximum Acceleration: 1061 g's