Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15662	**Temperature:**	22.4 °C
Model:	KICHER PR	**Humidity:**	30%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

411.3 mv/5000g
(82.3 µv/g)
R^2: 0.999969 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 16 2026

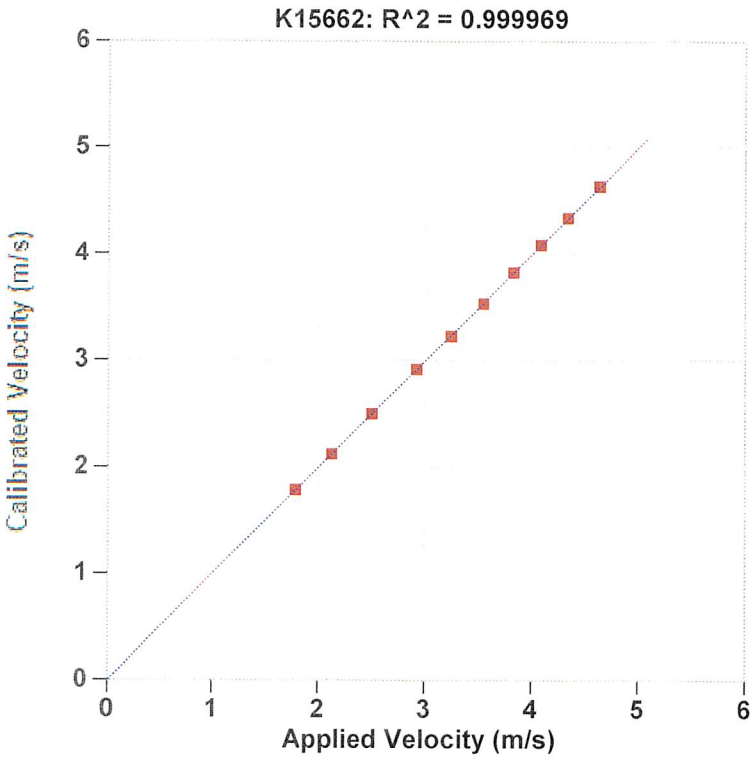

Reference Velocity	S/N K15662 Velocity
m/s	m/s
1.786	1.789
2.129	2.126
2.509	2.505
2.925	2.921
3.244	3.235
3.547	3.541
3.832	3.834
4.085	4.087
4.338	4.341
4.629	4.638

Maximum Acceleration: 1049 g's