Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15666	**Temperature:**	22.4 °C
Model:	KICHER PR	**Humidity:**	30%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

422.7 mv/5000g
(84.5 µv/g)
R^2: 0.999978 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 16 2026

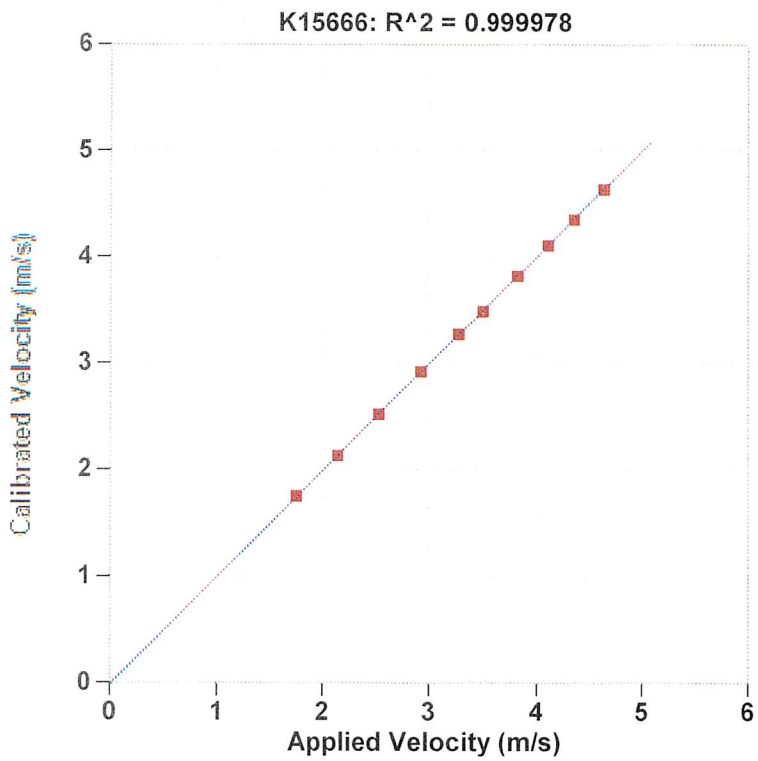

Reference Velocity	S/N K15666 Velocity
m/s	m/s
1.748	1.758
2.143	2.141
2.532	2.527
2.923	2.926
3.271	3.275
3.494	3.490
3.823	3.823
4.108	4.109
4.359	4.355
4.636	4.638

Maximum Acceleration: 1051 g's