Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15667	**Temperature:**	22.4 °C
Model:	KICHER PR	**Humidity:**	30%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

394.9 mv/5000g
(79.0 µv/g)
R^2: 0.999985 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 9 2026

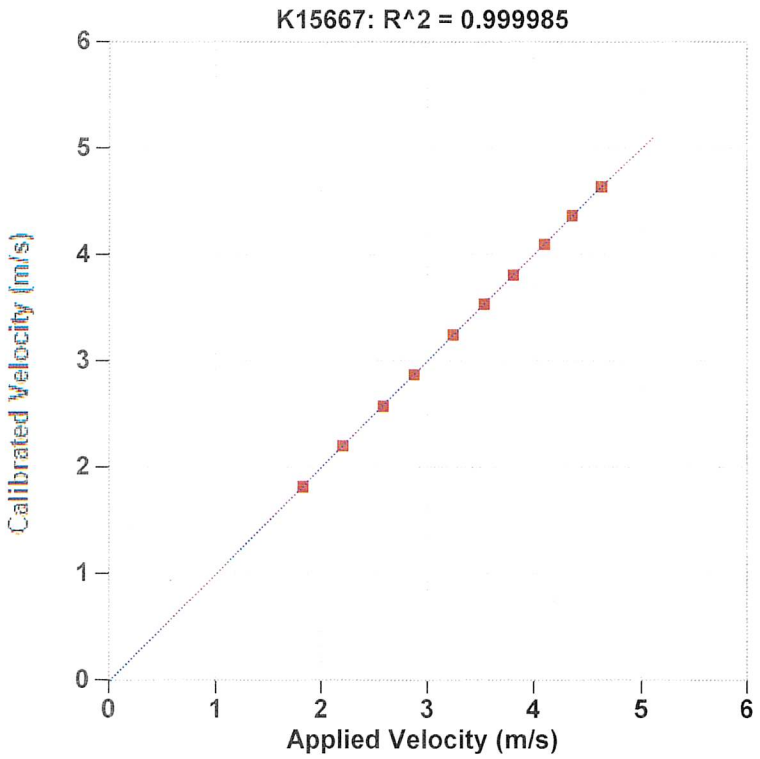

Reference Velocity	S/N K15667 Velocity
m/s	m/s
1.822	1.822
2.206	2.205
2.585	2.576
2.873	2.874
3.246	3.250
3.538	3.538
3.812	3.812
4.102	4.101
4.367	4.370
4.643	4.643

Maximum Acceleration: 1052 g's