Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15672	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	45%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

420.0 mv/5000g
(84.0 µv/g)
R^2: 0.999960 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

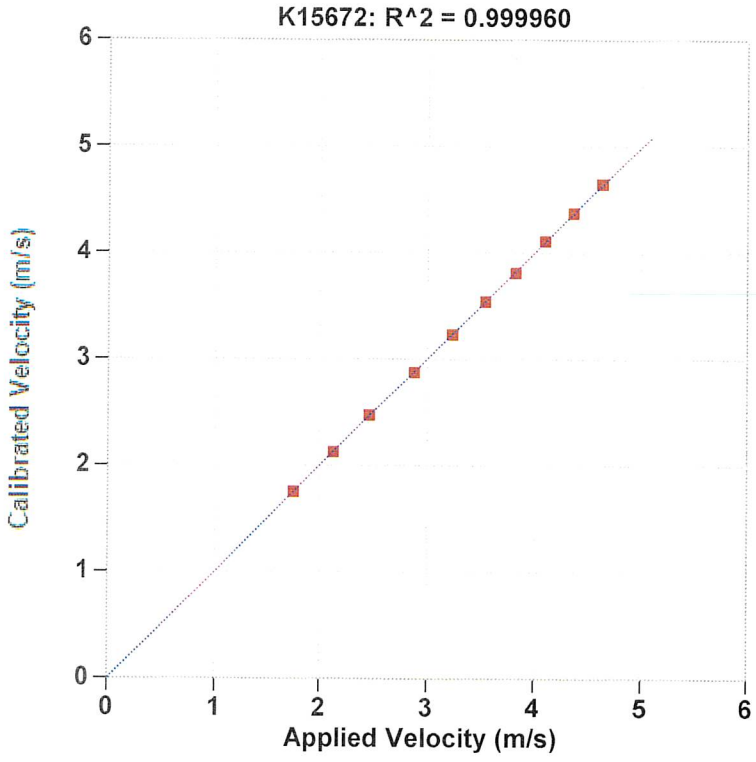

Reference Velocity	S/N K15672 Velocity
m/s	m/s
1.750	1.749
2.129	2.123
2.468	2.471
2.873	2.871
3.230	3.229
3.540	3.538
3.824	3.810
4.099	4.106
4.369	4.370
4.637	4.646

Maximum Acceleration: 1049 g's