Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15673	**Temperature:**	22.9 °C
Model:	KICHER PR	**Humidity:**	45%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

426.0 mv/5000g
(85.2 µv/g)
R^2: 0.999935 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

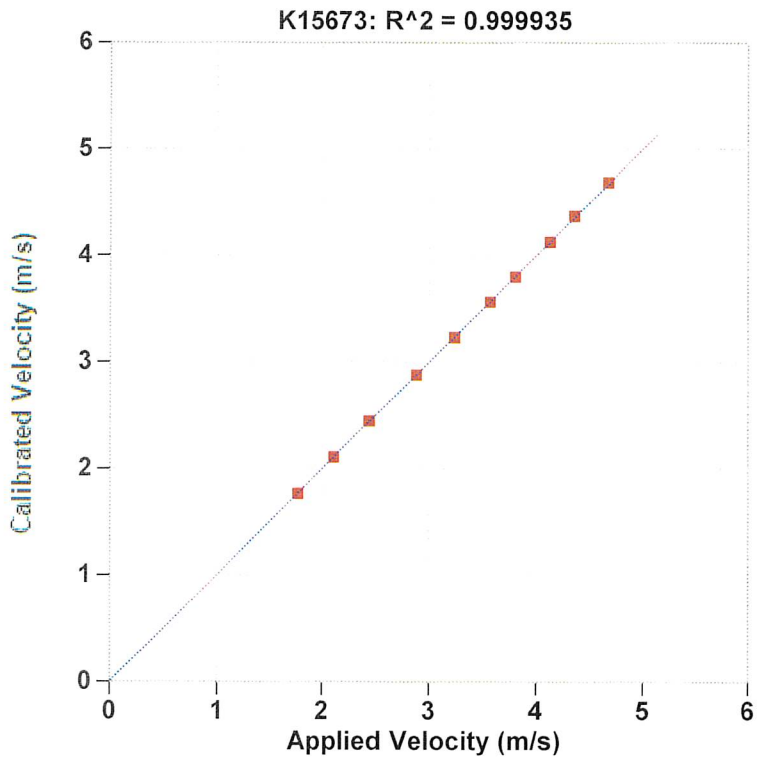

Reference Velocity	S/N K15673 Velocity
m/s	m/s
1.765	1.763
2.112	2.105
2.442	2.444
2.878	2.874
3.235	3.228
3.570	3.563
3.805	3.796
4.127	4.125
4.358	4.369
4.666	4.680

Maximum Acceleration: 1055 g's