Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15674	**Temperature:**	23.1 °C
Model:	KICHER PR	**Humidity:**	45%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

382.1 mv/5000g
(76.4 µv/g)
R^2: 0.999984 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 6 2026

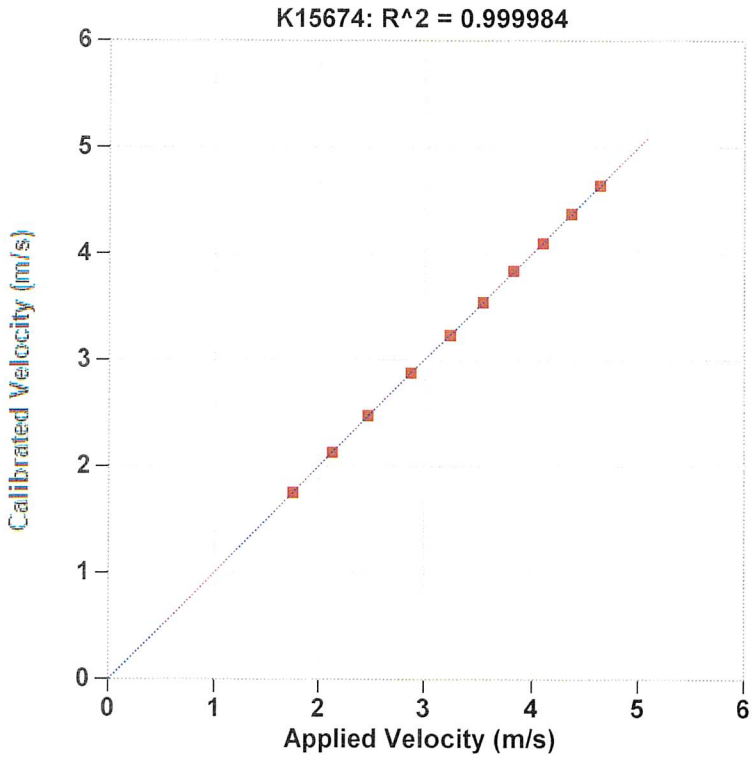

Reference Velocity	S/N K15674 Velocity
m/s	m/s
1.750	1.749
2.129	2.129
2.468	2.472
2.873	2.874
3.230	3.229
3.540	3.539
3.824	3.831
4.099	4.091
4.369	4.369
4.637	4.636

Maximum Acceleration: 1049 g's