Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K15676	**Temperature:**	22.4 °C
Model:	KICHER PR	**Humidity:**	30%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	85382! 958 g's/volt	**Cal on:**	24Nov2025
Ref Acc 2:	85363! 1000 g's/volt	**Cal on:**	14Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

377.5 mv/5000g
(75.5 µv/g)
R^2: 0.999976 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: NOV 0 9 2026

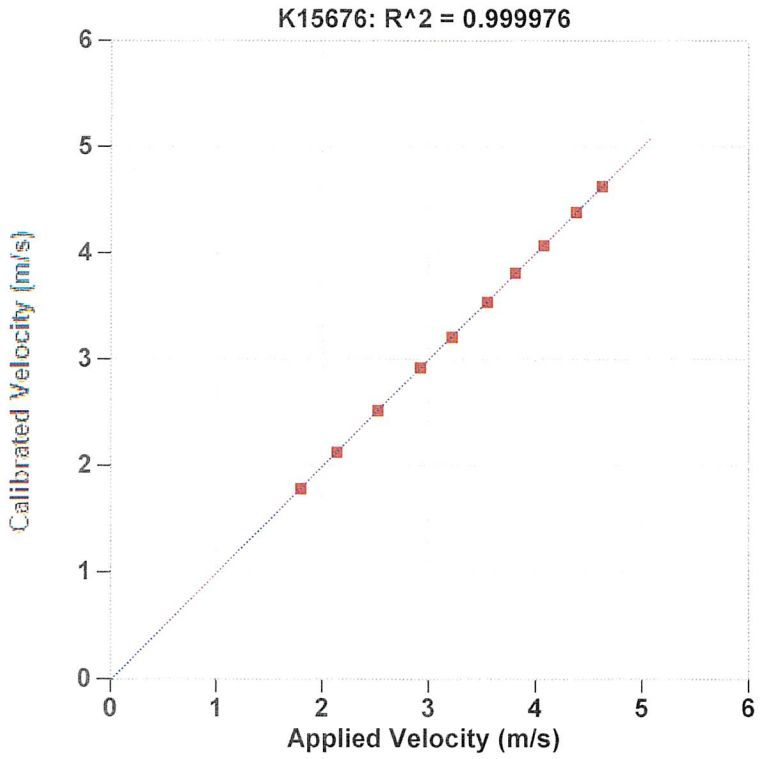

Reference Velocity	S/N K15676 Velocity
m/s	m/s
1.796	1.791
2.137	2.132
2.528	2.523
2.926	2.926
3.220	3.214
3.546	3.546
3.813	3.818
4.079	4.077
4.385	4.390
4.630	4.634

Maximum Acceleration: 1051 g's