
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: N563
PDI Gage Factor: 144.8
Mean Linear Correlation Coefficient: 0.999523

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2104.1	-4.464	393.7	0.830
-1607.6	-3.422	721.8	1.426
-1141.7	-2.424	1049.9	2.075
-708.7	-1.471	1410.8	2.785
-275.6	-0.578	1778.2	3.518
91.9	0.197	1994.8	3.957

Calibration Curve

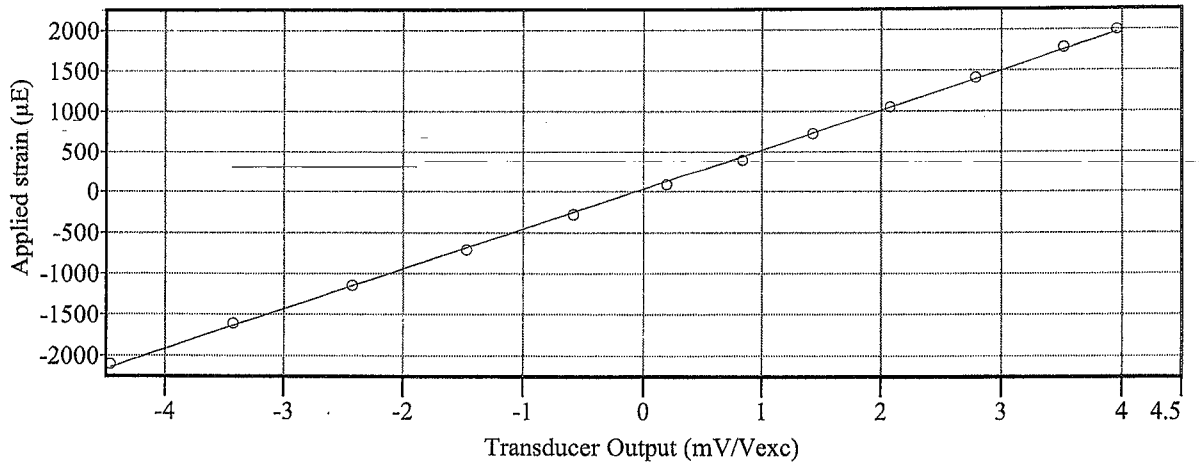

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: N563
Calibration Date: 7/23/2026 1:13:34 PM
Calibration valid 2 years

Pile Dynamics, Inc.