
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: S428
PDI Gage Factor: 140.4
Mean Linear Correlation Coefficient: 0.999942

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-1608.1	-3.402	660.4	1.315
-1210.8	-2.564	1034.0	2.077
-830.1	-1.743	1388.3	2.805
-406.4	-0.883	1738.3	3.503
-33.7	-0.134	1996.3	4.020
300.4	0.566		

Calibration Curve

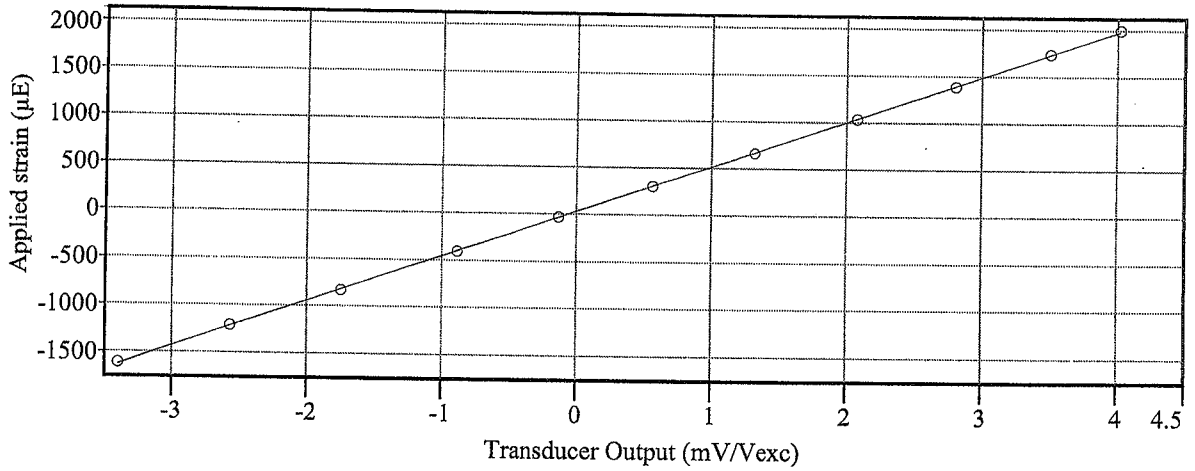

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: S428

Calibration Date: 10/23/2026 7:43:50 AM

Calibration valid 2 years

Pile Dynamics, Inc.