
Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: V884
PDI Gage Factor: 91.4
Mean Linear Correlation Coefficient: 0.999901

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2009.4	-6.275	575.1	1.980
-1562.6	-4.867	989.0	3.274
-1071.6	-3.314	1390.2	4.502
-647.2	-1.964	1772.2	5.666
-254.5	-0.684	1992.1	6.322
143.6	0.604		

Calibration Curve

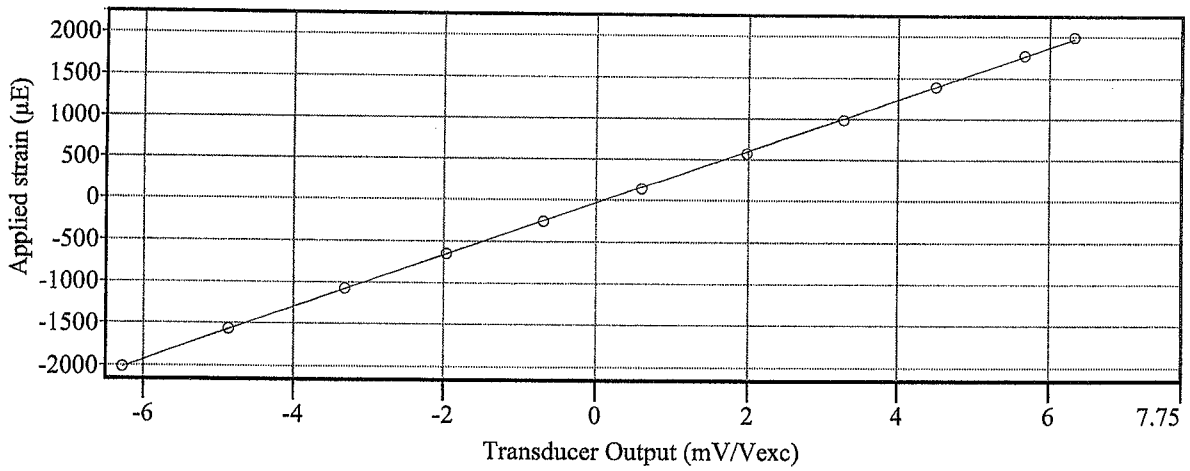

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: V884

Calibration Date: 10/26/2026 10:00:21 AM

Calibration valid 2 years

Pile Dynamics, Inc.